








Product Information

Understand information for simpler and easier operation

- A.LCD display area
- B.setting
- C.MODE
- D.detecting area
- E.Down
- F.Up
- G.testing key
- H.Battery cover

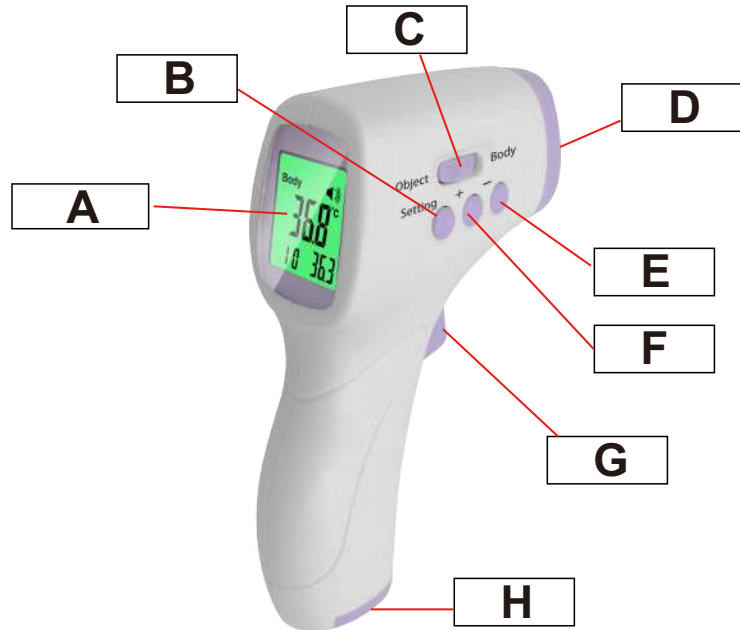

For People	Unlimited Crowds	Memory Array	32 Units
Measurement Method	Non-Contact	Power Supply	DC.3V (AAA*2)
Measurement Site	Forehead	GB Size	93x53x165mm
Measuring Distance	1-3cm	Weight	136g
Measuring Range	Body: 30.0°C~43.0°C	Max. Allowable Error	35°C~42.0°C (±0.2°C) Others (±0.3°C)

Package Information	Amount : 50PCS/ Carton	Carton Size: 483*348*285mm	
	Weight : 9.3KG/ Carton	Carton Volume: 0.0481CBM)	
Cabinet Type	20' GP	40' GP	40' HC/HQ
Packing Number	580CTNS	1160CTNS	1400CTNS
The Total Amount	29000PCS	58000PCS	70000PCS
Internal Dimensions	5.898*2.3 52*2.385	12.032*2.352*2.385	12.032*2.352*2.69
External Dimensions	6.058*2.438*2.591	12.192*2.438*2.591	12.192*2.438*2.896
Volume(Actually Fit)	33.1 (28CBM)	67.5(58CBM)	76.2(68CBM)

LST

Shenzhen LST Technology Co.,Ltd.

HOTLINE: 400-096-8018

WWW.LST-LAB.COM

Certificate of Compliance

Certificate No. : LST200378039E-2
Applicant : Hunan JRT Medical Devices Co.,Ltd
Applicant Address : Room 304, Building B5, Dreamworks, No. 1, Lantian North Road, Xingsha Industrial Base, Changsha Economic and Technological Development Zone, Hunan Province, China
Manufacturer : Hunan JRT Medical Devices Co.,Ltd
Manufacturer Address : Room 304, Building B5, Dreamworks, No. 1, Lantian North Road, Xingsha Industrial Base, Changsha Economic and Technological Development Zone, Hunan Province, China
Product M/N : Non-contact Infrared Thermometer
: JRT-023
: JRT-016,JRT-017,JRT-018,JRT-019,JRT-029
Trademark : JR TYL
Test Standard : EN 60601-1-2:2015
(CISPR 11:2015;IEC 61000-3-2:2014;IEC 61000-3-3:2013;
IEC 61000-4-2:2008;IEC 61000-4-3:2006;IEC 61000-4-4:2012;
IEC 61000-4-5:2014;IEC 61000-4-6:2013;IEC 61000-4-8:2009;
IEC 61000-4-11:2004)

The EUT described above has been tested by us with the listed standards and found in compliance with the council MDD directive 93/42/EEC. It is possible to use CE marking to demonstrate the compliance with this MDD Directive. It is only valid in connection with the test report number: LST200378039ER-2.

CE



Manager

Issue Date: Apr. 07, 2020

LST

Shenzhen LST Technology Co., Ltd.

HOTLINE: 400-096-8018

WWW.LST-LAB.COM

Certificate of Compliance

Certificate No. : LST200378039F-2
Applicant : Hunan JRT Medical Devices Co.,Ltd
Applicant Address : Room 304, Building B5, Dreamworks, No. 1, Lantian North Road, Xingsha Industrial Base, Changsha Economic and Technological Development Zone, Hunan Province, China
Manufacturer : Hunan JRT Medical Devices Co.,Ltd
Manufacturer Address : Room 304, Building B5, Dreamworks, No. 1, Lantian North Road, Xingsha Industrial Base, Changsha Economic and Technological Development Zone, Hunan Province, China
Product : Non-contact Infrared Thermometer
M/N : JRT-023
JRT-016, JRT-017, JRT-018, JRT-019, JRT-029
Trademark : JRTYL
Test Standard :

The submitted sample of the equipment has been tested and found to comply with the following standards:

- FCC Part 15 B
- ANSI C63.4:2014

This verification is part of the full test report(s) and should be read in conjunction with it. The referred test report(s) show that the product complies with standard(s) recognized as giving presumption of compliance with the essential requirements in the specified FCC standard. This Verification does not imply assessment of the production of the product. It is only valid in connection with the test report number: LST200378039FR-2.



Manager

Issue Date: Apr. 07, 2020



CERTIFICATION OF REGISTRATION

To:

Hunan Jrt Medical Devices Co., Ltd
Room 304, Building B5, Dreamworks, No.1, Lantian North Road, Xingsha
Industrial Base, changsha Economic and Technological Development Zone,
Changsha, Hunan, 410000, CHINA

is registered and has listed the following medical device with **the U.S. Food and Drug Administration(FDA)** :

Owner/Operator Number : 10070673

Listing Number: D393624

Product Code : FQZ

Product : Forehead Infrared Thermometer

Model(s) : JRT-018, JRT-016, JRT-017, JRT-023, CW-88

Date Of Registration Status: 2020

Registrar Corp will confirm that such registration remains effective upon request and presentation of this certificate until the end of the year stated above, unless said registration is terminated after issuance of this certificate. Registrar Corp makes no other representations or warranties, nor does this certificate make any representations or warranties to any person or entity other than the named certificate holder, for whose sole benefit it is issued. This certificate does not denote endorsement or approval of the certificate-holder's device or establishment by **the U.S. Food and Drug Administration(FDA)**. Registrar Corp assumes no liability to any person or entity in connection with the foregoing.

Pursuant to 21 CFR 807.39, "Registration of a device establishment or assignment of a registration number does not in any way denote approval of the establishment or its products. Any representation that creates an impression of official approval because of registration or possession of a registration number is misleading and constitutes misbranding."

The U.S. Food and Drug Administration(FDA) does not issue a certificate of registration, nor does the U.S. Food and Drug Administration recognize a certificate of registration. Registrar Corp is not affiliated with **the U.S. Food and Drug Administration(FDA)**



Chief Engineer / Zaccheo Lee

Issued: Apr. 18, 2020

Validity Period: 2020-12-31



Establishment Registration & Device Listing Website :

<https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfRL/rl.cfm>